

Fitting guide for AirFit F10



 Remove the elbow from the mask by pressing the side buttons and pulling it out.



• Take off the lower headgear straps and hold the cushion to the face. Align the bottom with the crease of the chin and the top with



- Undo the fastening tabs on the upper headgear straps.
- Adjust both straps evenly until the mask feels stable, then reattach the tabs.



- Connect device air tubing to the elbow, then attach the elbow to the mask by pressing in the side buttons, then push it into the mask.
- Turn on the device so it blows air.
- The patient now lies down to make any final adjustments if required.



• Bring the lower straps below the ears and


each side of the frame.

loop the headgear into the lower hooks on

- Undo the tabs on the upper headgear straps. • Reposition both straps evenly, only enough
- so a seal is achieved, then reattach the tabs.
- The mask is now ready to use.



Additional options



Note: For more details, refer to the AirFit F10 user guide.

Optimal cushion positioning



Align the bottom of the cushion with the crease of the chin, and the top of the cushion with the corner of the eye.

* ResMed internal study of existing ResMed patients, conducted between July 25 and September 4, 2013 comparing their ResMed traditional full face mask with AirFit F10.

Distributed by ResMed Corp, 9001 Spectrum Center Boulevard, San Diego, CA 92123 USA +1 858 836 5000 or 1 800 424 0737 (toll free). AirFit, SoftEdge and Spring Air are trademarks of ResMed. SoftEdge is registered in the U.S. Patent and Trademark Office. Specifications may change without notice. © 2014 ResMed. 1017251/3 2014-05

- the corner of the eye.
 - Then pull the headgear over the head.



- Adjust the lower headgear straps evenly until the mask feels stable.
- The fitting should be firm yet comfortable. Do not over-tighten.











AirFit F10 sits on the nose at, or below, eye level.

Full face benefits in a compact size

ResMed's AirFit[™] F10 full face mask is part of ResMed's AirFit range – the right fit for you. Its lightweight, streamlined design enhances comfort and ease-of-use, while its headgear and frame work in synergy, to deliver the same performance and stability you have grown to trust in a ResMed traditional full face mask.

Superior comfort

AirFit F10's sleek, lightweight design gives patients a clear line of sight so they can read, watch TV or even wear glasses while wearing the mask. In fact, 75% of patients found AirFit F10 to be more comfortable than their current ResMed traditional full face mask.*

Proven performance

The dual-wall Spring Air[™] cushion provides a secure seal for better performance. When asked about AirFit F10's seal and stability, the majority of patients we spoke to, told us that it outperformed their ResMed traditional full face mask.*

Ease-of-use


The mask's four-part design makes it easy for you to demonstrate and for patients to take apart, clean and reassemble. Its intuitive design seamlessly integrates into your patient's bedtime routine.






Quick to fit, easy-to-use


A recent ResMed study showed that the majority of patients could be set up and fitted with AirFit F10 in under two minutes.* Thanks to its built-in simplicity and four-part design, the mask is also easier for patients to use helping to reduce call backs and save time. You can be sure AirFit F10 is the right fit for your business.



AirFit F10 components

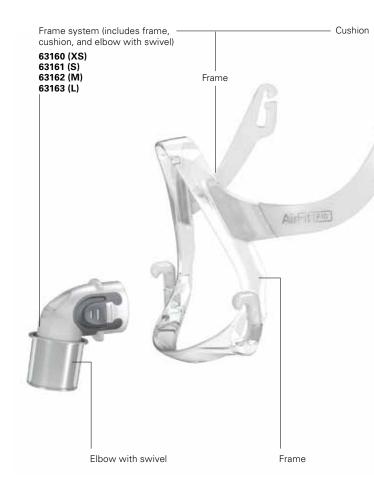


AirFit F10 features and benefits

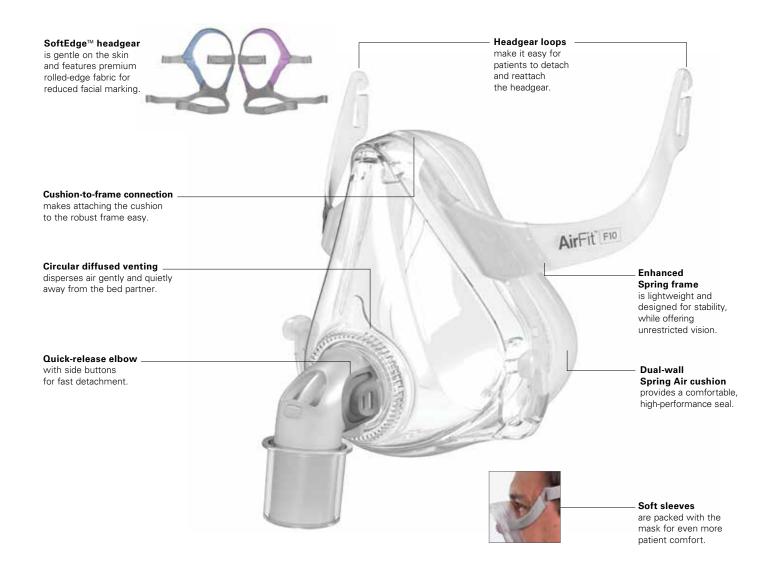

Note: For more details, refer to the AirFit F10 user guide.

Product codes (Complete mask system)

AirFit F10: Small	63101
AirFit F10: Medium	63102
AirFit F10: Large	63103
AirFit F10 for Her: X-Small	63139
AirFit F10 for Her: Small	63140
AirFit F10 for Her: Medium	63141

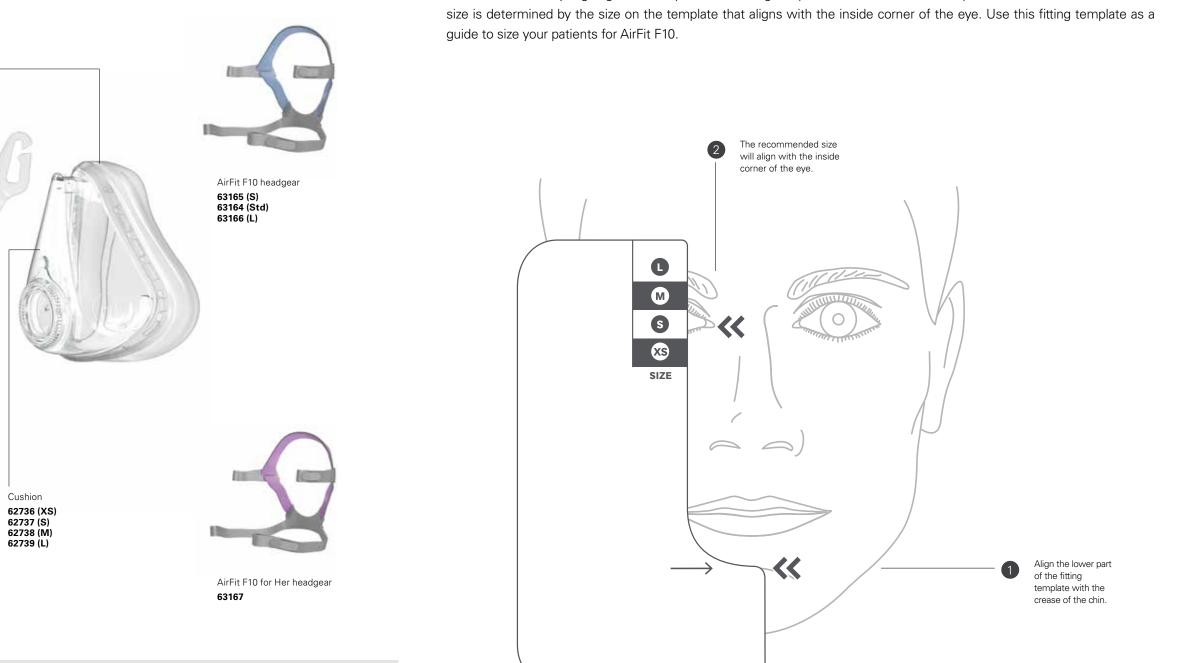

AirFit F10 sizing tips

AirFit F10 is sized by aligning the lower part of the fitting template with the crease of the patient's chin. The recommended

In this example, the recommended size would be Small.

* Combined responses of those expressing a preference in an independent patient survey in the USA, UK, Germany, France & Australia, from September 2012. Visit www.Res

Cushion



Useful information

• Ensure the patient's mouth is relaxed and closed when sizing.